

UDC 612.795:612.014.422

Daton Medenou¹, Ivo Iliev², Basile Kounouhewa³,
Roland C. Houessouvo¹, A. Sèmiyou Adedjouma¹, Michael Adeyinka⁴

PHYSICO-MATHEMATICAL BASIS OF THE BIOLOGICAL IMPEDANCE STUDY — CASE OF THE ELECTRODERMAL ACTIVITY

¹ Laboratory of Electrotechnics and Telecommunications and Application Informatics,
Abomey Calavi University, Cotonou, Benin,

² Medical Technics Laboratory/Electronics Department, Technical University, Sofia, Bulgaria,

³ Technical Researches Faculty, Abomey Calavi University, Cotonou, Benin,

⁴ Biomedical Informatics Laboratory, The Netherlands

УДК 612.795:612.014.422

Д. Медену¹, И. Ильев², Б. Кунухева³, Р. С. Хуессуво¹, А. С. Адедюма¹, М. Адеинка⁴
ФИЗИКО-МАТЕМАТИЧЕСКИЕ ОСНОВЫ ИЗМЕРЕНИЙ БИОЛОГИЧЕСКОГО ИМПЕДАНСА
ПРИ ИССЛЕДОВАНИИ ЭЛЕКТРОДЕРМАЛЬНОЙ АКТИВНОСТИ

¹ Лаборатория электротехники, телекоммуникаций и прикладной информатики, Абомей
Университет Калави, Котона, Республика Бенин,

² Лаборатория медицинской техники, отдел электроники, Технический университет, Со-
фия, Болгария,

³ Факультет технических исследований, Абомей Университет Калави, Котона, Республика
Бенин,

⁴ Лаборатория биомедицинской информатики, Голландия

В исследовании исходили из необходимости определения зависимости реографических по-
казателей от объемного тока крови. Установлено, что вариабельность относительной величи-
ны объемного тока крови прямо пропорционально зависит от вариабельности показателей им-
педанса ($\Delta Z/Z$) в сегменте тканей тела, которые подлежат исследованию. Вместе с тем, наблю-
дается обратная пропорциональная зависимость вариабельности объемного тока крови от на-
турального логарифма общего импеданса ($\ln Z$).

Ключевые слова: электродермальная активность, формула Кубичека, измерение импеданса,
электроплетизмография.

UDC 612.795:612.014.422

Daton Medenou¹, Ivo Iliev², Basile Kounouhewa³, Roland C. Houessouvo¹, A. Sèmiyou Ade-
djouma¹, Michael Adeyinka⁴

PHYSICO-MATHEMATICAL BASIS OF THE BIOLOGICAL IMPEDANCE STUDY — CASE OF
THE ELECTRODERMAL ACTIVITY

¹ Laboratory of Electrotechnics and Telecommunications and Application Informatics, Abomey Ca-
lavi University, Cotonou, Benin,

² Medical Technics Laboratory/Electronics Department, Technical University, Sofia, Bulgaria,

³ Technical Researches Faculty, Abomey Calavi University, Cotonou, Benin,

⁴ Biomedical Informatics Laboratory, The Netherlands

Physical laws are reliable means of data processing techniques and particularly in medical engi-
neering. Specifically, biological objects demand a deep analysis of some regularly used formulas and
defined conditions, the lack of which will nurse some doubt as for the effectiveness of the formulae
particularly used in rheography. The basic formulas used in bioimpedance measurements are consi-
dered in this work. The insufficiency in the expression of blood volume change as a function of total resi-
stance (or biological impedance) relative to variation is being considered, while new expressions are
being proposed. For instance, it has been demonstrated that the relative blood volume variation $\Delta V/V$
is directly proportional to the relative impedance variation ($\Delta Z/Z$) within the body segment under investi-
gation and inversely proportional to the natural logarithm of the total impedance of the segment ($\ln Z$).

Key words: Electrodermal activity, Kubicek's formula, Impedance measurement, Electrople-
thysmography.



Introduction

The electromagnetic fields theory and methods of electric field analysis enable creating powerful non-invasive methods for the investigation of the activity of the heart, brain, skin, muscle, etc. by *potential measurement* (Electrocardiogram (ECG), Electromyogram (EMG), Electrooculogram (EOG), Electrogastrogram (EGG), Electrodermal Activity (EDA) by TARCHANOV [1] etc., or by *impedance measurement* (Electroplethysmogram (EPG), EDA) by FERRE [2] etc. The development of the latter group created powerful technical basis, methods and relatively simple mathematical process for calculating hemodynamic parameters [3–6] or the activity of sweat glands. It has been demonstrated by Fowles that the electrodermal response (EDR) is associated with the activity of sweat glands. A direct correlation exists between EDR and the activity of sweat gland. There are no EDR signals without the activity of sweat glands [7]. Concerning the impedance measurements, the mathematical formulas used are based on the laws of solid state of physics (for instance, Ohm's law) applicable for certain defined conditions which are met always proper to biological objects. The case of biological objects is considered with enough precautions regarding the application of this law. That is why some authors do not trust the formulae used in Electroplethysmography while others consider them as only useful for predicting hemodynamic parameters. In this article, a review of Ohm's law will be made while an update will be proposed in the first instance. Secondly, the application conditions of this law will be specified in biomedical engineering and finally the basic

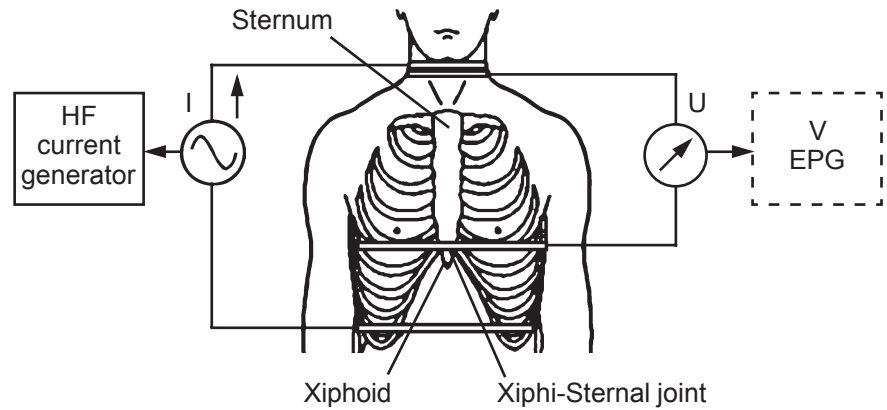


Fig. 1. Electroplethysmography measurement of cardiac impedance

Note. The impedance of the thorax is measured longitudinally by four electrodes band. A pair of external electrodes (an electrode is placed around the abdomen and other placed around the upper part of the neck). A pair of internal electrodes (an electrode is placed around the thorax at the level of the articulation between the xiphoid and the sternum, called the xiphoid articulation, and the other around the lower part of the neck). Source [15], reproduction.

formulas for impedance measurements will be reviewed.

Objective

The main objective in this work is to make a thorough review of the conditions of use of the laws of physics in engineering and particularly in medical engineering. To do this, we will:

- review Ohm's law in plethysmography and electrodermal activity;
- accentuate the weakness of the application of this law in the field of medical engineering;
- develop a new version of the application of this immutable law.

Problem

Measuring biological impedance reveals relative results when based on the current expression used in the calculation of hemodynamic parameters in rheography (fig. 1). Analysis demonstrates the need for an adjustment in the fundamental formulas based on Ohm's law and which are used in biological impedance measurements. Indeed, the voltage fall $U(V)$ on a conductor, through which a current runs is directly proportional to the resistance $R(\Omega)$ of the

conductor and the intensity $I(A)$ of this current.

$$U(V) = RI \quad (1)$$

The resistance R is an electrical property characteristic of the conductor, fig. 2, *a*, which depends on its geometric shape (dimensions), its homogeneity and its nature. This relationship is summarized in the following formula for every conductor and every shape:

$$R = \int \rho dl/ds \quad (2)$$

In this formula:

- ρ (Ωm) is the resistivity (specific resistance) of the material of the conductor and depends on some parameters as electron charge, carrier concentration, velocity, temperature, the charge of the conductor etc.;
- s (m^2) is the cross section of the conductor;
- l (m) is the length of the conductor.

When those parameters are constant in a solid conductor of length L defined as not very large, then the resistivity can be assumed to be constant with a relative uncertainty very low or negligible. Then the specific resistance is also constant.



Under these conditions, the formula of resistance can take the following simple form

$$R = \rho L/s = \rho L^2/sL \quad (3)$$

or

$$R = \rho L^2/V, \quad (4)$$

where $V \text{ (m}^3\text{)} = sL$ is the volume of the conductor.

The formula (4) is basical and is widely used in bioimpedance measurement. It was considered to be true and applicable to biological objects because of the early concept that human organism is electrically homogeneous. But this concept was later considered vague and/or only partially true [8], since it has been found that specific resistance of different tissues within human organism varies in large limits (as shown in the table 1) and together with the current frequency. Thus, it was found that the specific resistance (resistivity) of blood varies between $120\Omega\cdot\text{cm}$ and $180\Omega\cdot\text{cm}$ at current frequency of 500 Hz and between $118\Omega\cdot\text{cm}$ and $149\Omega\cdot\text{cm}$ at current frequency of 2.5 MHz. The conclusion was that the human organism is "relatively" homogeneously conductable. The same result was achieved by Nyboer [4]. Some years ago, Furthermore, Swanson confirmed that blood conductivity varies with the blood viscosity in blood vessels [14]. In spite of these results it has been accepted that certain average value of the blood specific resistance, which allows Ohm's law to be viable when measuring blood resistance or impedance. The blood specific resistance is still a function of the hematocrit. All that shows the relative character of the results when the expression (1) is used for the calculation of the hemodynamic parameters in rheography. Based on this analysis, an adjustment seems to be necessary in the fundamental

Table 1
The Resistivities of Some Tissues in the Body

Tissue	$\rho[\Omega\text{m}]$	Remarks
Brain	2.2	gray matter white matter average
	6.8	
	5.8	
Cerebro-spinal fluid	0.7	
Blood	1.6	Hct = 45
Plasma	0.7	
Heart muscle	2.5	longitudinal transverse
	5.6	
Skeletal muscle	1.9	longitudinal transverse
	13.2	
Liver	7	—
Lung	11.2	—
	21.7	
Fat	25	—
Bone	177	longitudinal circumferential radial (at 100 kHz)
	15	
	158	
	215	

Note. With Hct = Hematocrit (%). Source: [9–13].

formulas used in biological impedance measurements.

Materials and Methods

They are based on the reformulation of basic expressions of

rheography. In order to get more accurate and convenient rheomatics expressions, the calculation of parameters, data analysis and the blood resistance in a given body segment should be considered to be parallel with the resistance of the remainder of that segment (fig. 2, a, b, c, d).

In that figure, R_0 and R are the total resistance of the segment at moment t_0 (respectively at moment t), R_b , R_t and ΔR_b are respectively blood resistance, the resistance of the remainder tissues of the segment and the variation in blood resistance following the change ΔV in the blood volume V .

Within the segment the variation in the total resistance is noted ΔR as:

$$\Delta R = R - R_0 \quad (5)$$

From fig. 2, we have:

$$\Delta R_b = -RR_0/\Delta R \quad [21-23] \quad (6)$$

R_b is the resistance of the blood.

With reference to the expression (4) we obtain:

$$\Delta R_b = \rho L^2/\Delta V \quad (7)$$

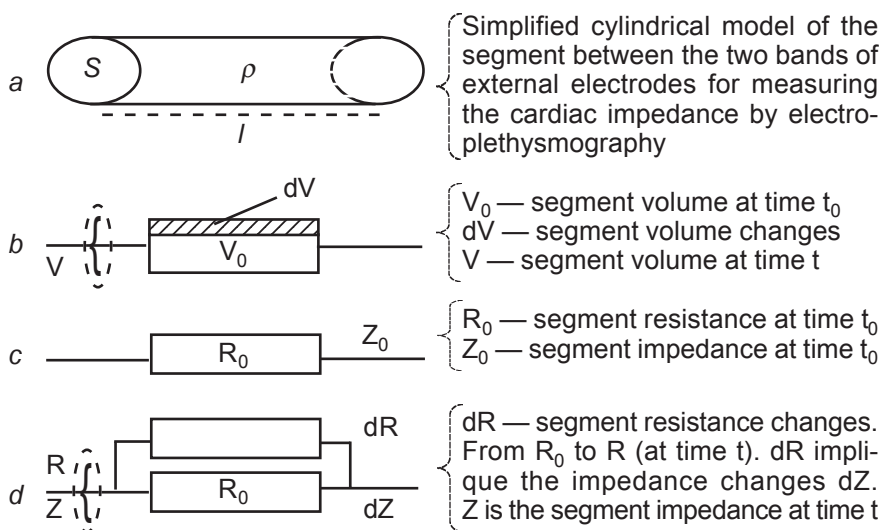


Fig. 2. Electric models of the body part under investigation

Note. R_0 and R are the segment total resistances with the blood at time t_0 and t . R_b , R_t and ΔR_b are respectively the blood resistance, other tissues in the segment and with changes of the blood resistance in accordance with changes in the blood volume.



Since only the blood volume has varied in the segment, the change in volume of the segment is also the change in blood volume thus:

$$\Delta V = \Delta V_b \quad (8)$$

It follows:

$$\Delta V = -\rho L^2/R_0 \cdot \Delta R/R \quad (9)$$

In case of elementary change in blood volume dV , we get

$$dV = -\rho L^2/R_0 \cdot dR/R \quad (10)$$

A solution of the expression (10) is

$$V = -\rho L^2/R_0 \cdot \ln(k \cdot R) \quad (11)$$

In this expression k is a coefficient (k normalizer in Siemens or $1/\Omega$), which expresses the constant of integration.

From the expressions (9) and (11) we get:

$$\Delta V/V = (\Delta R/R) \times 1/\ln(k \cdot R) \quad (12)$$

We note that this result is widely different from the usually used expression and that the discrepancy is certainly not noticed because of the approximations used in Electroplethysmogram (EPG).

Results

Application to electrodermal activity by FERE: Electrodermal activity (EDA or EDF) is a signal recorded at the surface of the skin and which reflects the psychophysiological state of the body. This activity can be recorded either as a potential (TARH-ANOFF method) or as a change in impedance (Method FERE). We use the skin series equivalent model — FERE model (fig. 3). It has been shown that only tissue resistivity is required and that the effect of electromagnetic propagation can be neglected [16; 18], except for a respiratory inductance plethysmography [19].

Since the series equivalent model is used and since the presence of inductance is not yet

accepted by numerous authors, between the impedance Z and the active resistance R we have the following relation:

$$Z = R(1 + 1/(RC\omega)^2)^{1/2} = \eta R \quad (13)$$

C is the capacity of the tissues within the segment. Since in bioimpedance measurements (EPG, EDA etc.) changes in active resistance R and in capacity C are small (absent some per cent) (Nyboer 1970), η is almost constant and may be calculated for each rheography and the body segment. Due to the reason explained above it may be accepted that the measured impedance Z is proportional to the active resistance R , thus:

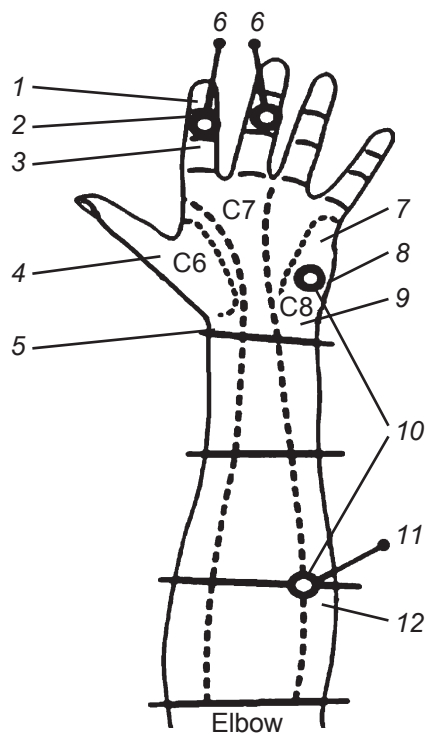


Fig. 3. Electrodes locations on the palm for measurement the resistance and potential of the skin. (Venables et Christie, 1980). Reproduction. Source [17]: 1 — distal phalanx; 2 — medial phalanx; 3 — proximal phalanx; 4 — thenar eminence; 5 — crease; 6 — bipolar placement (SC measurement); 7 — hepothernar eminence; 8 — active electrode; 9 — dermatomal distribution; 10 — unipolar placement (SC measurement); 11 — reference electrode; 12 — abraded site

$$|Z| = \eta R \quad (14)$$

The frequency f is related to the pulsation ω by the equation $\omega = 2\pi f$. Because the rheography works at a fixed frequency (selective), we can not expect the change in ω which could give rise to changes in η . Therefore $\Delta Z/Z = (\Delta R/R) \cdot (\Delta \eta/\eta)$.

From the expression (14) we may get:

$$\Delta Z/Z = \Delta R/R \quad (15)$$

In expression (12) when we replace $\Delta R/R$ by $\Delta Z/Z$ and we make a proper calibration of the measuring instrument, we obtain:

$$\Delta V/V = (\Delta Z/Z) \times 1/\ln(k/\eta Z) \quad (16)$$

The ratio k/η can be reduced to the unit from the calibration of the meter. Thus the final formula becomes:

$$\Delta V/V = (\Delta Z/Z) \cdot 1/\ln(Z) \quad (17)$$

Analysis

Discussion & Perspectives

This last formulation (17) is based on skin abrasion and can be used safely in all measurements of biological impedance variations related to changes in various flowing objects in the body (such as blood, lymph, sweat, etc.). This is helpful because the skin impedance varies for each individual and depends primarily on: the skin temperature, the surface and contact pressure, contact tension (force), the moisture condition and sweating of the skin, the time of passage of the electrical current, physiological state, the morphology of the individual and the contact points on the body.

We note that expression (12) is widely different from the usually used expression while the discrepancy remains certainly not noticed because of the approximations used in Electroplethysmogram (EPG).



It is necessary to have here a short discussion: in expression (4) ρ is the blood resistivity, the resistance R must be the blood resistance, so that V represents the blood volume, but in expression (12) R is the total resistance of the segment. All the formulas above concern only active resistance. However, current measurement is never a direct current because of the danger due to the faradic effect. So, in reality, it is rather the total resistance. However, many authors toggle from the active resistance to complex resistance (the impedance), replacing R by Z ! This requires a prior adjustment.

In impedance, the influence of plethysmography capacitance is reduced to minimum value by skin abrasion and the use of high frequencies (20 KHz to 200 KHz), but nonetheless the measured quantity is indeed impedance since reactive components are not completely cancelled.

The ratio k/η deserves special attention and can be reduced to the unit from the calibration of the meter. If $k/\eta < 1 > k/\eta$? In reality, the value to be assigned will depend on the scope and measurement conditions in each clinical specialty.

Regarding impedance, we want to know if the resistivity of the blood is not a function of other parameters in addition to the Hematocrit. Furthermore, we will also have to make an experimental phase to justify the approach.

In our opinion the results should provide further details in the calculation of cardiac parameters such as: cardiac output, heart rate, maximum frequency theoretical intracardiac hemodynamic, corrected QT interval, mean arterial pressure, cardiovascular risk, and valve area.

Conclusion

There are some difficulties in using certain formulas in the theory and practice of plethysmography (EPG) and in their applications to other biological impedance measurements (such as Electrodermal Activity). This shows the limitations and shortcomings of these formulas.

This work shows some inadequacy in the basic formulae used in impedance rheography measurement while at the same time proposing solutions without the aforementioned discrepancies. The proposed formulas are based on reliable physical basis, but they may not be considered as the final correction in the wide range (largely used formulas), but simply as a step in the research of universal solution to the insufficiency.

This formula contains two parameters, still undetermined k and h but with the practical conditions on the current frequency of measures for h and on the calibration of the meter for k .

Concluding therefore, our conclusion is a challenge to the engineers to determine these parameters, and more still, to the physicists who are looking for conditions, on which physical laws of matter could be based on medical objects.

REFERENCES

1. Tarchanoff J. (1889). Décharges électriques dans la peau de l'homme sous l'influence de l'excitation des organes des sens et de différentes formes d'activité psychique. *C. Soc. Biol.* (Paris) 41: 447-451.
2. Féré C. (1888). Note sur les modifications de la résistance électrique sous l'influence des excitations sensorielles et des émotions. *C. R. Soc. Biol.* (Paris) 5: 217-219.
3. Nyboer J. (1950). Electrical impedance plethysmography. *Circulat*; 2: 811-821.
4. Nyboer J. (1970). Electrorheometric properties of tissues and fluids.

Ann. New York Acad. Sciences; 2: 410-420.

5. Kubicek W.G., Patterson R.P., Wtsoe D.A. (1970). Impedance cardiography as non invasive method of monitoring cardiac function and others parameters of cardiovascular system. *Ann. New York Acad. Science*; 2: 724-732.

6. Stamboliev I.B., Penev H., Munshinski A. Method for determining some elements of impedance plethysmography (IPG) signals to be used in automatic. *Advances in Biomedical Measurement* Ed. E. Carson et al. Plenum Press 1988, 167-169.

7. Fowles D.C. (1986). The eccrine system and electrodermal activity. In *Psychophysiology*, ed. M.G.H. Coles, E. Donchin, S.W. Porges, Guilford Press, New York. P. 51-96.

8. Benjamin M.J., Schwan H., Kaay C.F., Hafkenschiel J.H. (1980). The electrical conductivity of living tissues. *Circulat*; 2 (3): 321-335.

9. Geddes L.A., Baker L.E. (1967). The specific resistance of biological material A compendium of data for the biomedical engineering and physiologist. *Med. Biol. Eng.*; 5: 271-293.

10. Barber D.C., Brown B.H. (1984). Applied potential tomography. *J. Phys. E.: Sci. Instrum.* 17:723-33. Epstein B.R., Foster K.R. (1983). Anisotropy as a dielectric property of skeletal muscle. *Med. & Biol. Eng. & Comput.*; 21 (1): 51-55.

11. Stuchly M.A., Stuchly S.S. (1984). Electrical properties of biological substance. In *Biological Effects and Medical Applications of Electromagnetic Fields*, ed. O.P. Gandhi, Academic Press, New York.

12. Stuchly M.A., Stuchly S.S. (1984). Electrical properties of biological substance. In *Biological Effects and Medical Applications of Electromagnetic Fields*, ed. O.P. Gandhi, Academic Press, New York.

13. Jaakko Malmivuo & Robert Plonsey. *Bioelectromagnetism — Principles and Applications of Bioelectric and Biomagnetic Fields*, New York Oxford, Oxford University Press, 1995. Version 2007.11.07; Section7. (<http://www.kenrico.com/media/bembook/> OU <http://www.bem.fi/book/07/07.htm>). (consulté le 10-09-2012).

14. Swanson D.K., Webster J.G. (1983). Errors in four electrode impedance plethysmography. *Med. & Biol. & Comput.*; 21: 674-680.

15. Jaakko Malmivuo & Robert Plonsey. *Bioelectromagnetism — Principles and Applications of Bioelectric and Bio-*



magnetic Fields, New York Oxford, Oxford University Press, 1995. Version 2007.11.07; Section 25. (<http://www.kenrico.com/media/bembook/> OU <http://www.bem.fi/book/25/25.htm>). (consulté le 10-09-2012).

16. John Wiley & Sons, Inc.. MEDICAL INSTRUMENTATION: application and design. John G. Webster, editor; 4th Edition (2009). Sec. 5, p. 207.

17. Jaakko Malmivuo & Robert Plonsey. *Bioelectromagnetism — Principles and Applications of Bioelectric and Biomagnetic Fields*, New York Oxford, Oxford University Press, 1995. Version 2007.11.07; Section 27. (<http://www.kenrico.com/media/bembook/> OU <http://www.bem.fi/book/27/27.htm>). (consulté le 10 -09-2012).

18. Jaakko Malmivuo & Robert Plonsey. *Bioelectromagnetism — Principles and Applications of Bioelectric and Biomagnetic Fields*, New York Oxford, Oxford University Press, 1995. Version 2007.11.07; Sous-Section 7.2.4 (<http://www.kenrico.com/media/bembook/> OU <http://www.bem.fi/book/07/07.htm>). (consulté le 10-09-2012).

19. Gandis G. Mazeika, Rick Swanson (2007). Respiratory Inductance Plethysmography An Introduction. Pro-Tech Services, Inc. www.pro-tech.com

20. Jia-Jung Wang, Wei-Chih Hu, Tsiar Kao, Chun-Peng Liu, Shih-Kai Lin (2011). Development of forearm impedance plethysmography for the minimally invasive monitoring of cardiac pumping function. *J. Biomedical Science and Engineering*; 4: 122-129. doi: 10.4236/

jbise.2011.42018 Published Online February 2011 (<http://www.SciRP.org/journal/jbise/>).

21. Stamboliev I.B., Medenou D. (1989). Influence of electrode of technic on EDA investigation. Conference, "Radiology Day, 7th May" Sofia. Conference. (in bulgarian).

22. Stamboliev I.B., Penev H., Munshinski A. Method for determining some elements of impedance plethysmography (IPG) signals to be used in automatic. *Advances in Biomedical Measurement*, ed. E. Carson et al. Plenum Press 1988, p. 167-169.

23. Medenou D. Enregistrement et analyse de l'activité électrodermale. Thèse Université Technique de Sofia. Sofia, 1990.

Submitted 6.06.2013

